



التاريخ : 16.7.2018

الرقم:


تنويه بخصوص مناقصة رقم MOH-GSD/MOFP/2018/123 " شراء وتوريد وتركيب

أجهزة طبية لمشروع تشطيب طوارئ مستشفى رفيديا - نابلس لصالح وزارة الصحة

بناء على بعض الاستفسارات التي وردتنا على المناقصة المذكورة اعلاه، مرفق لكم ملخص لاستفسارات الشركات على البندين (5 + 13) والردود عليها، ويعتبر هذا التنويه جزء من وثائق المناقصة ويجب على جميع الشركات ارفاقه مع كراسة المناقصة .

وتفضلوا بقبول فائق الاحترام،،،

المكلف بمهام نظام اللوازم العامة
رئيسة اللجنة للوازم العامة
16.7.2018



التاريخ :

الرقم:

الرد على استفسارات الخاصة بالمواصفات الفنية للبندين (البند رقم 5 + البند رقم 13)

نود توضيح ما يلي:

• البند رقم 5 (Digital x-ray machine) :

Attached is the AutoCad Drawing for the X-ray Room

• البند رقم 13 (Whole body Multi slice CT Scanner (128 slices)) :

1. Upgradable System:

Software upgrades that enhance existing applications, increase productivity & improve safety related issues should be provided by the vendor at no cost to the MOH till the functioning of the machine.

2. Injector Protocol:

No Change, Protocol Memory: around 50

3. Latest dose reduction techniques:

Quoted CT scanner models should have latest raw data / model based iterative reconstruction technique (MBIDR) launched by company used for low dose scanning, which should be offered as standard.

4. Independent work station:


The workstation software should be from original equipment manufacturer of the CT scan machine.

5. Under the warranty & CAMC:

Warranty period is extendable for the same down time period during warranty, in addition the company will pay for services outside for 4 emergency cases /day after Grace time (8days) during down time.


6. Attached is the AutoCad Drawing for the CT-SCAN Room

16/7/2018

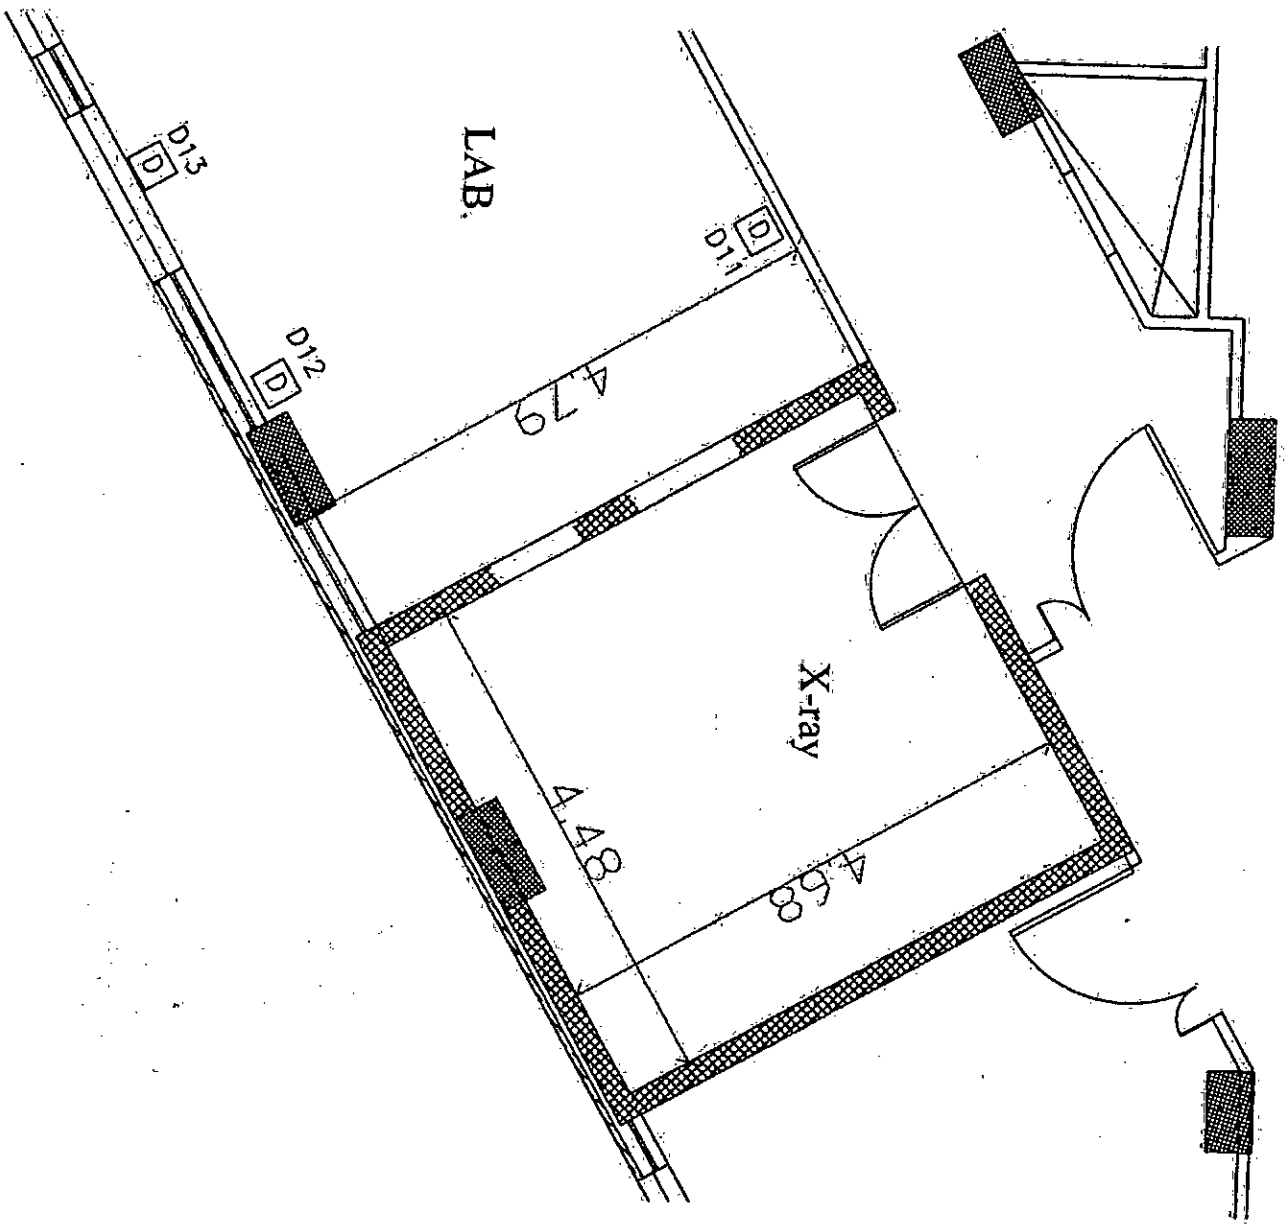

Rafedia X-ray = 21m²

11

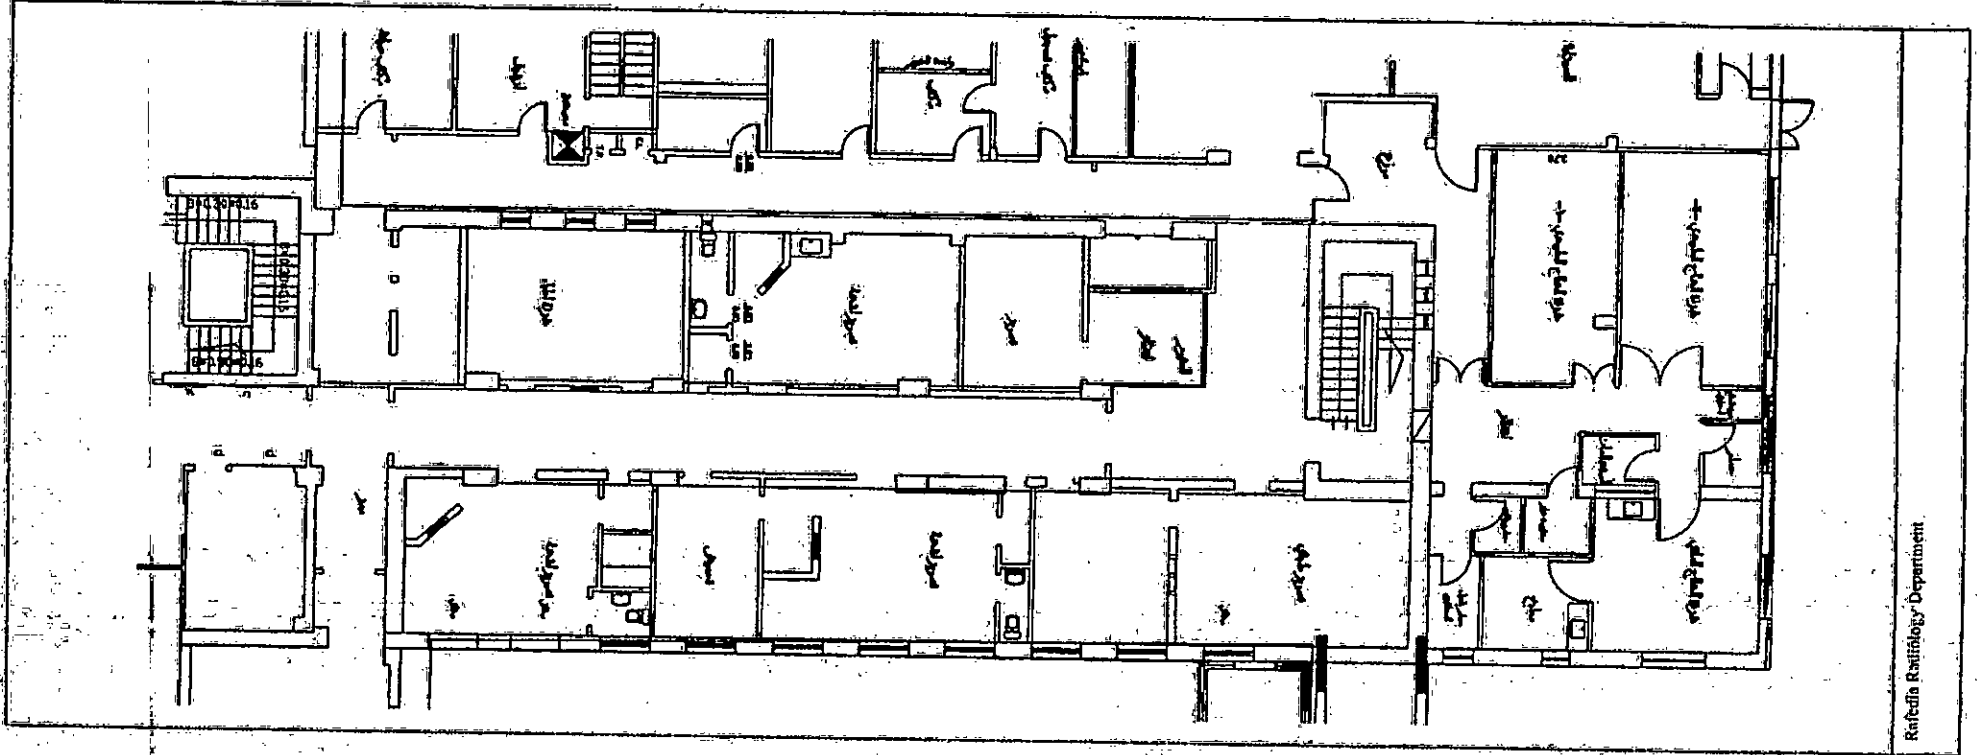

Rafedla Rafidology Department